

# Custom Labels

## Tailored To Your Operating Room Needs

**Codonics Safe Label System (SLS)** is a first-in-its-class solution that brings automation, compliance, and safety to the point of care. SLS is an "FDA-cleared" Class II medical device intended for safe and effective automatic verification of drug identity using barcode data from NDC and other drug vial UDI barcodes. The system enables the creation of compliant drug class color-coded ISO26825 and ASTM 4774 labels while adhering to TJC-MM & ISMP medication standards in alignment with ASA, APSP, and TJC medication safety guidance & goals to enhance medication safety. But syringe labeling is just the beginning.

**With SLS, facilities unlock powerful flexibility**—enabling **fully customized, on-demand labels** for IV lines, invasive monitors, patient samples, airway alerts, high-risk medications, and more. Whether you're managing a complex case in the OR or organizing high-acuity workflows in the ICU, SLS empowers your team to improve communication, reduce risk, and drive consistency across every touchpoint.

**Custom labels** are designed to match your hospital's unique clinical needs and environment.

- Clear, color-coded labels that improve communication a glance
- Durable design for high-demand clinical environments — won't smudge, curl, or peel
- Standardizes labeling across the OR and ICU — supporting safety, speed, and team communication



**Codonics SLS empowers facilities to enhance safety, efficiency, and compliance with fully customizable labeling solutions.**

For example, a "DIFFICULT INTUBATION" label can be printed and placed on a patient's forehead to alert clinicians of a complex airway case, or "GAUGE LABELS" can be used to clearly indicate the gauge size on an IV.



## Custom Labels Tailored To Your Operating Room Needs

### Antibiotics Labels for ICU

**Tygacil**  
Prepared: 10/18/2024 18:14 By: Q  
Expires: \_\_\_\_\_

**Maxipime**  
Prepared: 10/18/2024 18:10 By: Q  
Expires: 10/19/2024 18:10

**Meropenem**  
Prepared: 10/18/2024 18:15 By: Q  
Expires: \_\_\_\_\_

**Dalacin**  
Prepared: 10/18/2024 18:15 By: Q  
Expires: \_\_\_\_\_

**Zavicefta**  
Prepared: 10/18/2024 18:10 By: Q  
Expires: 10/19/2024 18:10

**Ceftriaxone**  
Prepared: 10/18/2024 18:15 By: Q  
Expires: \_\_\_\_\_

**Tazocin**  
Prepared: 10/18/2024 18:16 By: Q  
Expires: \_\_\_\_\_

**ANTIBIOTIC**  
Prepared: 10/18/2024 18:14 By: Q  
Expires: \_\_\_\_\_

**PENICILIN**  
Prepared: 10/18/2024 18:29 By: Q  
Expires: \_\_\_\_\_

### Blood Gas Analysis

**ABG ANALYSIS**  
Prepared: 10/18/2024 18:35 By: Q  
Expires: \_\_\_\_\_

**VBG ANALYSIS**  
Prepared: 10/18/2024 18:35 By: Q  
Expires: \_\_\_\_\_

### Colleague Alert Labels

**Exp:.....**  
Prepared: 10/18/2024 18:40 By: Q  
Expires: \_\_\_\_\_

**ICP**  
Prepared: 10/18/2024 18:38 By: Q  
Expires: \_\_\_\_\_

**NOT FOR CLINICAL USE**  
Prepared: 10/18/2024 18:40 By: Q  
Expires: \_\_\_\_\_

**DRAINS**  
Prepared: 10/18/2024 18:31 By: Q  
Expires: \_\_\_\_\_

**Surgivac**  
Prepared: 10/18/2024 18:27 By: Q  
Expires: \_\_\_\_\_

**ALCOHOL 70%**  
Prepared: 10/18/2024 18:32 By: Q  
Expires: \_\_\_\_\_

**DIFFICULT INTUBATION**  
Prepared: 10/18/2024 18:38 By: Q  
Expires: \_\_\_\_\_

**UVC**  
Prepared: 10/18/2024 18:11 By: Q  
Expires: \_\_\_\_\_

**AMINOSOL 20%**  
Prepared: 10/18/2024 18:29 By: Q  
Expires: 10/19/2024 18:29

**LOW K+**  
Prepared: 10/18/2024 18:09 By: Q  
Expires: \_\_\_\_\_

**UROBAG**  
Prepared: 10/18/2024 18:31 By: Q  
Expires: \_\_\_\_\_

**LA**  
Prepared: 10/18/2024 18:35 By: Q  
Expires: \_\_\_\_\_

### Combination Drugs for ICU

**Dopamine & Dobutamine**  
Prepared: 10/18/2024 18:39 By: Q  
Expires: 10/19/2024 18:39

**Dormicum & Fentanyl**  
Prepared: 10/18/2024 18:39 By: Q  
Expires: 10/19/2024 18:39

**Electrolyte+Aminosol**  
Prepared: 10/18/2024 18:11 By: Q  
Expires: \_\_\_\_\_

# Custom Labels Tailored To Your Operating Room Needs

## Department Labels

<p><b>Oncology</b></p> <p>Prepared: 10/18/2024 18:09      By: Q Expires: _____</p>	<p><b>ADULT OR</b></p> <p>Prepared: 10/18/2024 18:41      By: Q Expires: _____</p>	<p><b>Anesthesia Dept.</b></p> <p>Prepared: 10/18/2024 18:39      By: Q Expires: _____</p>
<p><b>AOR PERFUSION DEPT</b></p> <p>Prepared: 10/18/2024 18:43      By: Q Expires: _____</p>	<p><b>Perfusion DEPT.</b></p> <p>Prepared: 10/18/2024 18:40      By: Q Expires: _____</p>	<p><b>Nebulizer Set</b></p> <p>Prepared: 10/18/2024 18:44      By: Q Expires: _____</p>
<p><b>RA</b></p> <p>Prepared: 10/18/2024 18:35      By: Q Expires: _____</p>	<p><b>Humidifier</b></p> <p>Prepared: 10/18/2024 18:43      By: Q Expires: _____</p>	

## Diluent Labels: Custom labels can be created to reflect any diluent type, the percentage of that diluent, or the specific amount used.

<p><b>Ringer Lactate</b></p> <p>Prepared: 10/18/2024 18:36      By: Q Expires: _____</p>	<p><b>Glucose 17.5%</b></p> <p>Prepared: 10/18/2024 18:13      By: Q Expires: _____</p>	<p><b>50% DEXTROSE</b></p> <p>Prepared: 10/18/2024 18:34      By: Q Expires: 10/19/2024 18:34</p>
<p><b>1/2 DNS</b></p> <p>Prepared: 10/18/2024 18:33      By: Q Expires: _____</p>	<p><b>Glucose 20%</b></p> <p>Prepared: 10/18/2024 18:13      By: Q Expires: _____</p>	<p><b>NS 0.45%</b></p> <p>Prepared: 10/18/2024 18:33      By: Q Expires: _____</p>
<p><b>LIPOFUNDIN 20%</b></p> <p>Prepared: 10/18/2024 18:36      By: Q Expires: _____</p>	<p><b>Glucose 25%</b></p> <p>Prepared: 10/18/2024 18:13      By: Q Expires: _____</p>	<p><b>3% NS</b></p> <p>Prepared: 10/18/2024 18:33      By: Q Expires: _____</p>
<p><b>Glucose 5%</b></p> <p>Prepared: 10/18/2024 18:11      By: Q Expires: _____</p>	<p><b>Glucose 30%</b></p> <p>Prepared: 10/18/2024 18:13      By: Q Expires: _____</p>	<p><b>NS (Flush) 0.9%</b></p> <p>Prepared: 10/18/2024 18:33      By: Q Expires: _____</p>
<p><b>Glucose 7.5%</b></p> <p>Prepared: 10/18/2024 18:12      By: Q Expires: _____</p>	<p><b>40% Glucose</b></p> <p>Prepared: 10/18/2024 18:31      By: Q Expires: _____</p>	<p><b>D5NS</b></p> <p>Prepared: 10/18/2024 18:28      By: Q Expires: 10/24/2024 18:28</p>
<p><b>Glucose 10%</b></p> <p>Prepared: 10/18/2024 18:12      By: Q Expires: _____</p>	<p><b>Glucose 50%</b></p> <p>Prepared: 10/18/2024 18:14      By: Q Expires: _____</p>	<p><b>D51/2NS</b></p> <p>Prepared: 10/18/2024 18:28      By: Q Expires: _____</p>
<p><b>Glucose 12.5%</b></p> <p>Prepared: 10/18/2024 18:12      By: Q Expires: _____</p>	<p><b>10% DEXTROSE</b></p> <p>Prepared: 10/18/2024 18:33      By: Q Expires: 10/19/2024 18:33</p>	<p><b>LR</b></p> <p>Prepared: 10/18/2024 18:28      By: Q Expires: _____</p>
<p><b>Glucose 15%</b></p> <p>Prepared: 10/18/2024 18:13      By: Q Expires: _____</p>	<p><b>20% DEXTROSE</b></p> <p>Prepared: 10/18/2024 18:33      By: Q Expires: 10/19/2024 18:33</p>	<p><b>SALINE 0.45%</b></p> <p>Prepared: 10/18/2024 18:28      By: Q Expires: 10/24/2024 18:28</p>

Label colors and categories shown here are samples only, reflecting practices from various hospitals. They are not recommendations. Custom labels can be created to meet your facility's specific needs and use cases.

## Custom Labels Tailored To Your Operating Room Needs

### Gauge Labels

**14 Gauge**  
Prepared: 10/18/2024 18:38 By: Q  
Expires: 10/20/2024 18:38

**16 Gauge**  
Prepared: 10/18/2024 18:38 By: Q  
Expires: 10/20/2024 18:38

**18 Gauge**  
Prepared: 10/18/2024 18:38 By: Q  
Expires: 10/20/2024 18:38

**20 Gauge**  
Prepared: 10/18/2024 18:38 By: Q  
Expires: 10/20/2024 18:38

**22 Gauge**  
Prepared: 10/18/2024 18:39 By: Q  
Expires: 10/20/2024 18:39

**24 Gauge**  
Prepared: 10/18/2024 18:39 By: Q  
Expires: 10/20/2024 18:39

### High Alert / High Risk Labels for ICU

**High Alert**  
Prepared: 10/18/2024 18:08 By: Q  
Expires: \_\_\_\_\_

**MgSO4 & Lidocaine20%**  
Prepared: 10/18/2024 18:09 By: Q  
Expires: \_\_\_\_\_

**Na Bicarbonate**  
Prepared: 10/18/2024 18:37 By: Q  
Expires: \_\_\_\_\_

**High Risk**  
Prepared: 10/18/2024 18:08 By: Q  
Expires: \_\_\_\_\_

**Potassium Phosphate**  
Prepared: 10/18/2024 18:37 By: Q  
Expires: \_\_\_\_\_

**Sodium Chloride**  
Prepared: 10/18/2024 18:37 By: Q  
Expires: \_\_\_\_\_

**HIGH K+**  
Prepared: 10/18/2024 18:09 By: Q  
Expires: \_\_\_\_\_

**Magnesium Sulphate**  
Prepared: 10/18/2024 18:37 By: Q  
Expires: \_\_\_\_\_

**Calcium Gluconate**  
Prepared: 10/18/2024 18:37 By: Q  
Expires: \_\_\_\_\_

**Isupril**  
Prepared: 10/18/2024 18:19 By: Q  
Expires: \_\_\_\_\_

**ULTIVA**  
Prepared: 10/18/2024 18:27 By: Q  
Expires: \_\_\_\_\_

**Insulin**  
Prepared: 10/18/2024 18:27 By: Q  
Expires: \_\_\_\_\_

**IMMUNOGLOBULIN**  
Prepared: 10/18/2024 18:19 By: Q  
Expires: \_\_\_\_\_

**Precedex**  
Prepared: 10/18/2024 18:25 By: Q  
Expires: \_\_\_\_\_

**TRIDIL**  
Prepared: 10/18/2024 18:24 By: Q  
Expires: \_\_\_\_\_

**Nipride**  
Prepared: 10/18/2024 18:24 By: Q  
Expires: \_\_\_\_\_

**CORDARONE**  
Prepared: 10/18/2024 18:19 By: Q  
Expires: 10/19/2024 18:19

**Primacor**  
Prepared: 10/18/2024 18:18 By: Q  
Expires: \_\_\_\_\_

**Angiomax**  
Prepared: 10/18/2024 18:18 By: Q  
Expires: \_\_\_\_\_

## Custom Labels Tailored To Your Operating Room Needs

### Lines + Drains Labels

**Peritoneal Cath**

Prepared: 10/18/2024 18:33 By: Q  
Expires: \_\_\_\_\_

**CENTRAL LINE**

Prepared: 10/18/2024 18:30 By: Q  
Expires: \_\_\_\_\_

**Catheter Line**

Prepared: 10/18/2024 18:31 By: Q  
Expires: 10/21/2024 18:31

**EPIDURAL CATHETER**

Prepared: 10/18/2024 18:30 By: Q  
Expires: 10/21/2024 18:30

**EPIDURAL**

Prepared: 10/18/2024 18:32 By: Q  
Expires: \_\_\_\_\_

**Plural Tube**

Prepared: 10/18/2024 18:27 By: Q  
Expires: \_\_\_\_\_

**FOLEY'S CATHETER**

Prepared: 10/18/2024 18:30 By: Q  
Expires: \_\_\_\_\_

**PA**

Prepared: 10/18/2024 18:37 By: Q  
Expires: \_\_\_\_\_

**PERIPHERAL LINE**

Prepared: 10/18/2024 18:32 By: Q  
Expires: 10/21/2024 18:32

**UAC**

Prepared: 10/18/2024 18:11 By: Q  
Expires: \_\_\_\_\_

**Arterial**

Prepared: 10/18/2024 18:31 By: Q  
Expires: \_\_\_\_\_

**Electrolyte**

Prepared: 10/18/2024 18:34 By: Q  
Expires: 10/21/2024 18:34

**CVP**

Prepared: 10/18/2024 18:31 By: Q  
Expires: \_\_\_\_\_

**D5LR**

Prepared: 10/18/2024 18:28 By: Q  
Expires: 10/19/2024 18:28

**Mediastinal Tube**

Prepared: 10/18/2024 18:34 By: Q  
Expires: 10/21/2024 18:34

**IVF(N.S 0.9%)**

Prepared: 10/18/2024 18:30 By: Q  
Expires: \_\_\_\_\_

**IVF (DNS)**

Prepared: 10/18/2024 18:32 By: Q  
Expires: \_\_\_\_\_

**PPI Infusion - LOSEC**

Prepared: 10/18/2024 18:25 By: Q  
Expires: \_\_\_\_\_

**IVF(5% Dextrose)**

Prepared: 10/18/2024 18:32 By: Q  
Expires: \_\_\_\_\_

**NGT Feed**

Prepared: 10/18/2024 18:32 By: Q  
Expires: 10/19/2024 18:32

**Symdex Infusion**

Prepared: 10/18/2024 18:26 By: Q  
Expires: \_\_\_\_\_

**AMINOSOL 10%**

Prepared: 10/18/2024 18:29 By: Q  
Expires: 10/19/2024 18:29

**LIPOFUNDIN 10%**


Prepared: 10/18/2024 18:28 By: Q  
Expires: 10/19/2024 06:28

**HEPARIN Infusion**


Prepared: 10/18/2024 18:27 By: Q  
Expires: \_\_\_\_\_

## Custom Labels Tailored To Your Operating Room Needs

### Organizational Labels: Tag bins and drawers throughout the perioperative area

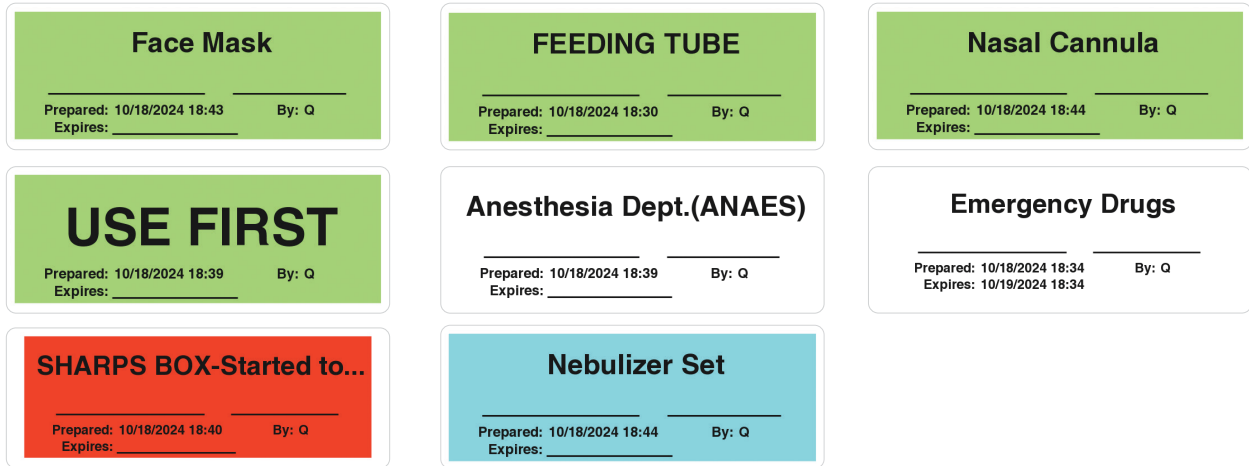

### Service / Maintenance Labels for OR & ICU

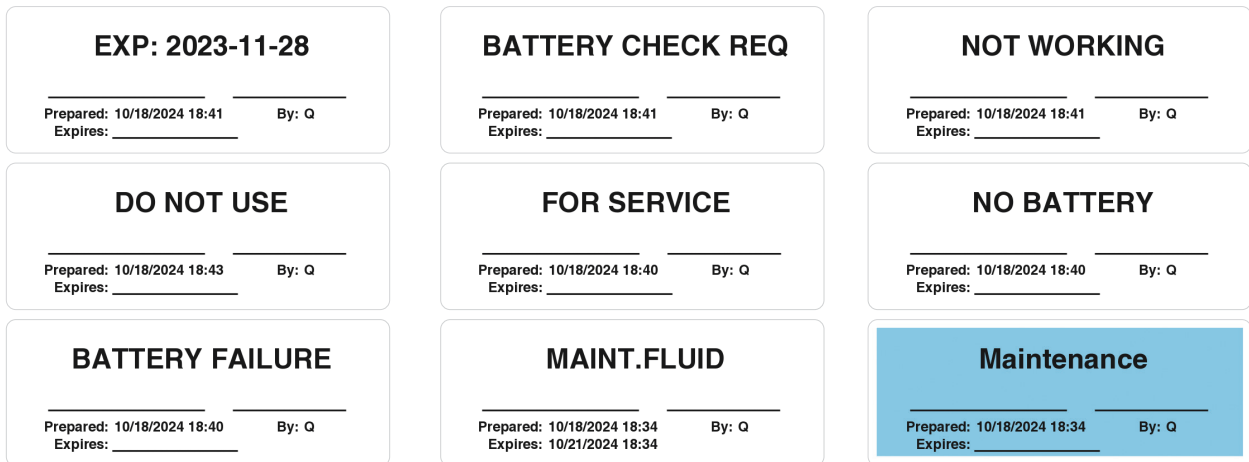

Label colors and categories shown here are samples only, reflecting practices from various hospitals. They are not recommendations. Custom labels can be created to meet your facility's specific needs and use cases.

Call Codonics today at **800.444.1198** or visit [www.codonics.com](http://www.codonics.com) for more information.



**Caution:** Federal law restricts this device to sale by or on the order of a physician or other practitioner licensed by the law of the state in which the device is used. The SLS device must be in the possession of a licensed practitioner for use in the course of professional practice. All registered and unregistered trademarks are the property of their respective owners. Specifications subject to change without notice.  
 Patents: [www.codonics/ip/patents](http://www.codonics/ip/patents) Printed in the U.S.A. Copyright © 2025 Codonics Inc 08/2025.  
 Codonics Safe Label System (SLS) is an FDA-cleared Class II medical device.

17991 Englewood Drive  
 Middleburg Heights, OH 44130 USA  
 +1.440.243.1198  
 +1.440.243.1334 Fax  
[info@codonics.com](mailto:info@codonics.com)  
[www.codonics.com](http://www.codonics.com)

#### GLOBAL WEBSITES

Latin America: [www.codonics.lat](http://www.codonics.lat) | Middle East: [www.codonics.ae](http://www.codonics.ae) | Africa: [www.codonics.fr](http://www.codonics.fr) | China: [www.codonics.cn](http://www.codonics.cn)

900-917-001.03